

Instruction for use

## **MFD-57**

Automatic Blood Pressure Monitor



### 1. INTRODUCTION

Thank you for purchasing the B.Well Wrist Blood Pressure Monitor MED-57. Designed for convenient and easy operation, this device provides fast and reliable measurement of systolic and diastolic blood pressure as well as heart rate using the oscillometric measurement method.

The MED-57 is a fully automatic, digital, wrist blood pressure measuring device.

Intended use: The Blood Pressure Monitor MED-57 including accessories is a non-invasive blood pressure measurement system intended to measure the diastolic and systolic blood pressures and pulse rate of an adult individual by using the oscillometric

### **Application area:** for use by medical professionals or at home.

### Important advantages of MED-57:

- Large display with backlight. Up-to-date Intellect Active technology uses oscillometric measurement during inflation for quick, precise and gentle
- Memory of 30 measurements. Average of the last 3 measurements.
- Traffic Light Indication according to European Society of Hypertension (ESH).
- The Pulse Arrhythmia Detection technology.
- Date and Time
- For wrist circumference of 13,5-21,5 cm.


#### 2. CLASSIFICATION OF BLOOD PRESSURE VALUES Table for classifying blood pressure values (mmHg) according to European Society of Hypertension (ESH)

Range	Systolic blood pressure	Diastolic blood pressure	Measures
Grade 3: severe hypertension	Higher or equal to 180	Higher or equal to 110	Urgently seek medical advice!
Grade 2: moderate hypertension	160-179	100-109	Consult your doctor immediately
Grade 1: mild hypertension	140-159	90-99	Consult your doctor
High normal	130-139	85-89	Consult your doctor
Normal	Lower than 130	Lower than 85	Self-check
Optimal	Lower than 120	Lower than 80	Self-check

**•• NOTE:** Show the measured values to your doctor. Never use the results of your measurements to change the doses of drugs prescribed by your doctor.

## 3. CONTENTS AND DISPLAY INDICATORS

Model MED-57



M Memory Symbol ■ Indication of blood pressure level

- Pulse Arrhythmia Detection symbol ▼ Heart Beat Symbol
- Self-adjustment before measuremen Batteries are running out Low battery symbo 28:88 Date and time



## 4. CONTRAINDICATION

Do not use the device if there is a skin surface damage on the wrist. It is inappropriate for people with serious arrhythmia to use this device.

## 5. PRECAUTIONS

- 1. Read all of the information in the instruction for use before 2. Stay still, calm and rest for 5 minutes before blood pressure
- 3. The cuff should be placed at the same level as your heart. 4. During measurement, neither speak nor move your body and arm. Motion, trembling, shivering may affect the measurement
- 5. Measuring on the same wrist for each measurement (left wrist usuallv).
- 6. Please always relax about 5 minutes between measurements to allow the blood circulation in your arm to recover. Prolonged over-inflation (cuff pressure exceed 300 mmHg or maintained above 15 mmHg for longer than 3 minutes) of the bladder may
- cause ecchymoma of your arm. 7. Consult your physician if you have any doubt about below cases: 7.1. The application of the cuff over a wound or inflammation
- 7.2. The application of the cuff on any limb where intravascular access or therapy, or an arterio-venous (A-V) shunt, is
- 7.3. The application of the cuff on the arm on the side of a 7.4. Simultaneously used with other monitoring medical
- equipments on the same limb;
- 7.5. The usage by a person with a cardiac pacemaker. The device does not affect the cardiac pacemaker. However, if there is a serious arrhythmia or a low pulse, the measurement results may be inaccurate.
- 8. The device would not apply to the patients with poor peripheral circulation, noticeably low blood pressure, or low body

temperature (there will be low blood flow to the measurement position).

- 9. The device would not apply to the patients who use artificial heart and lung (there will be no pulse).
- 10. Consult your physician before using the device for any of the following conditions: common arrhythmias such as atrial or ventricular premature beats or atrial fibrillation, arterial sclerosis, poor perfusion, diabetes, pre-eclampsia, renal desieses.
- 11. The patient can be an intended operator
- 12. Swallowing batteries and/or battery fluid can be extremely dan gerous. Keep the batteries and the unit our of the reach of children and disabled persons.
- 13. If you are allergic to plastic/rubber, please don't use this device. 14.  $\triangle$  This digital automatic blood pressure monitor is designed for adults. The device is not intended for use on neonates, children or pregnant women (clinical testing has not been conducted on neonates, children or pregnant women). Consult your physician or other health care professionals before use on older children.
- 15. Do not use this unit in a moving vehicle.
- 16. Blood pressure measurements determined by this monitor are equivalent to those obtained by a trained observer using the cuff/stethoscope auscultation method, within the limits prescribed by the American National Standard Institute, Electronic or automated sphygmomanometers.
- 17. Information regarding potential electromagnetic or other interference between the blood pressure monitor and other devices together with advice regarding avoidance of such interference please see part ELECTROMAGNETIC COMPATIBILITY INFORMATION.
- 18. Please do not use the cuff other than supplied by the manufacturer, otherwise it may cause biocompatible hazard and might result in measurement error.
- 19. 

  The monitor might not meet its performance specifications or cause safety hazard if stored or used outside the specified temperature and humidity ranges in specifications.
- 20. Delease do not share the cuff with other infective person to avoid cross-infection.
- 21. Please note that changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.
- 22. This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following
- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver. Connect the equipment into an outlet on a circuit different. from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician

## 6. SETUP AND OPERATING PROCEDURES


### 6.1. Battery loading

- a. Open battery cover at the back of the monitor.
- Load two "AAA" size batteries. Please pay attention to polarity. c. Close the battery cover.
- d. Once you install the battery, in the OFF mode the LCD will
- display year (2018). You must adjust date and time (see section 6.2).
- △ If the LCD displays battery symbol 🗓 batteries are finishing.
- Please replace all batteries with new ones. △ After the LCD displays battery symbol ☐ the monitor cannot
- open. Please replace all batteries with new ones. △ Rechargeable batteries are not suitable for this monitor.
- △ Remove the batteries if the monitor will not be used for a
- month or more to avoid relevant damage of battery leakage △ Avoid the battery fluid to get in your eyes. If it should get in your eyes, immediately rinse with plenty of clean water and
- contact a physician. △ Make sure the battery cover is intact and not damaged before installing the battery.

The monitor, the batteries and the cuff, must be disposed of according to local regulations at the end of their usage.

## 6.2. Date and time adjustment

- a. Once you install the battery, in the OFF mode the LCD will display year (2018). See picture 2-1.
- b. Press the "M" button to increase the number. Press and hold the "M" button for more than 3 second, the number will increase
- c. After the year is set, press the "Time" button to confirm and proceed to month adjustment. Month number will start blinking. See picture 2-2.



d. Set the month (by pressing the "M" button to increase the value), then press the "Time" buttor

e. Repeat the steps above to set the day, hour and minute. See picture 2-3.

f. After the adjustment is finished, press the "Time" button. Date and time adjustment is completed, the device will enter the OFF mode. Now when the device is turned off, the LCD displays current date and time. If you need to change it, press and hold the "Time" button for 3 seconds. The device will switch to date and time adjustment mode.


When replacing the batteries, the date and time of the last


① **NOTE:** Sound signals might be turned off. To turn it off, press "Start" and "Time" buttons simultaneously for 3 seconds. The LCD will display ON, then OFF. Pelease the buttons. Now sound signals are turned off. To turn it on again, repeat the above steps and select ON. 6.3. Applying the cuff

## a. Place the cuff around a bare wrist 1-2 cm

measurement is saved.

above the wrist joint on the palm side of the wrist.





c. The cuff must be neither too tight nor too loose. At the same time,

 Avoid eating, smoking as well as all forms of exertion directly before the measurement. All these factors influence the measurement result. Try and find time to relax by sitting in an armchair in a quiet atmosphere for about five to ten minutes before the measurement.

Measure always on the same arm.

 Attempt to carry out the measurements regularly at the same time of day, since the blood pressure changes during the course

### Body posture during measurement

Be seated with your feet flat on the floor, and don't cross your legs.

The first way to measure

flat surface such as a desk or table. b. Place something under your arm (for example, the monitor storage bag) so that the middle of the cuff was at the level of the heart. Make sure that the cuff is not pressed by anything.

a. Place palm upside in front of you on a

## The second way to measure

a. Use the free hand to take the elbow of the arm with the blood pressure monitor.

- Place the arm with the monitor so that the palm of the arm would be next to the opposite shoulder, and the monitor – at the level of the heart
- Make sure that you see the display of the monitor. Relax your wrist joint and wrist (do not move your wrist forward or back, do not clench into a fist)

#### Common sources of error:

- Movement during measurement
- The monitor is not at the level of the heart • The cuff does not fit you in size

## 6.5. Taking your blood pressure reading

a. After applying the cuff and your body is in a comfortable position, press the "START" button. All display characters are shown for self-test (Picture 5-1). Please contact the service center if any segment is missing on

□ MONTH-DAY **38**÷88



Picture 5-2

- b. Then the monitor inflates the cuff and carries out the measurement. Finally the blood pressure and pulse rate will be calculated and displayed on the LCD screen. Irregular heartbeat symbol (if any) will blink on the screen.
- c. After measurement, the monitor will turn off automatically after 1 minute of no operation. Alternatively, you can press the "START" button to turn off the monitor manually
- d. During measurement, you can press the "START" button to turn off the monitor manually.

① **NOTE**: Please consult a health care professional for interpretation of pressure measurements.

## 6.6. Guest measurement mode

Guest measurement mode is used for single blood pressure measurement of another person. The measurement results are not

stored in the memory in this mode Press and hold the "Start" button for more than 3 seconds until date and time will disappear from LCD, then release the button. The device will start measurement.

The measurement result will be displayed on LCD.

## 6.7. Pulse Arrhythmia Detection

#### Appearance of the Pulse Arrhythmia Detection Symbol 4 means that a certain pulse irregularity was detected during the measurement. In this case, the result can vary from your

actual blood pressure that's why you should rest for 15 minutes and repeat the measurement The appearance of symbol 4/4 is accompanied by a sound signal As a rule this is not a cause for concern; however, if the symbol appears more frequently, we recommend you inform your doctor The monitor does not replace the cardiological examination, but it

### allows you to detect the arrhythmia even in early stages. 6.8. Traffic Light Indication


The colored bars on the left-hand edge of the display show you the range within which the indicated blood pressure values lies. Depending on the height of the bar, the readout value is either within the normal (green), borderline (yellow and orange) of danger (red) range. If the values of systole and diastole fall into two different categories (e.g. systole in the High normal category and diastole in the Normal category), the graphical classification on the device always shows the higher category (e.g. High). The classification corresponds to the 6 ranges in the Table as defi ned by the ESH and described on the table of the point 2. The recommendations of the European Society of Hypertension (ESH) allow to diagnose and treat the hypertension more effectively and do not contradict World Health Organization recommendations. Please note that these standard values serve only as a general guideline, as the individual blood pressure varies in different people and different age groups etc., it is important to consult your doctor regularly for advice.



#### 6.9. The average of last three measurements. To use the average pressure and pulse calculation function.

take 3 consecutive measurements at 1-3 minutes intervals. All 3 measurements will be stored in the device memory To view the average pressure and pulse, press the "Memory" button when the device is off. The LCD will display the total number of saved measurements first (picture 9-1). Then the "A" symbol and the average value of last

three measurements of systolic, diastolic pressure and pulse will be displayed (picture 9-2)




Due to the constant fluctuation of blood pressure, the result obtained in this way is more reliable than the single measurement result. Average measurement should be recorded regularly in the blood pressure diary.

 $\ensuremath{\textcircled{1}}$   $\ensuremath{\textbf{NOTE}}$  the result of average measurement is not stored in device memory and updates with every new measurement

#### 6.10. Saved measurements display a. To view saved measurement results press the "M" button while

the device is turned off.



b. The LCD will display the total number of saved results first

- (picture 10-1) c. Then the LCD will display the average of last three
- measurements (picture 10-2). d. Then the result, date, time and level on the pressure scale of last measurement will be displayed (at number 1, picture 10-3, 10-4). Irregular heartbeat symbol (if any) will blink at
- the same time e. Press the "M" button repeatedly to review the results measured previously (pictures 10-5, 10-6).
- By pressing the "M" button again, you can view the previous neasurement results, from the latest to the earlier. If you press and hold the "M" button for more than 2 seconds, the values will scroll faster and automatically.
- g. When displaying the stored results, the monitor will turn off automatically after 1 minute of no operation. You can also press the "Start" button to turn off the monitor manually. When the memory reaches 30 stored results, the older one will be deleted after new measurement

## 6.11. Deleting measurements from the memory

To delete all measurements, press and hold the "M" button for 5 seconds and release it when "CL" symbol is displayed (picture 11).



Picture 11 Press the "M" button once more to confirm. 3 beep signals will notify that results were successfully deleted.

The device will turn off automatically after 1 minute of no operation. You can also press the "Start" button to turn off the device manually.

Selective measurement result deletion is not provided

## 6.12. Technical alarm description

The monitor will show 'HI' or 'Lo' as technical alarm on LCD with no delay if the determined blood pressure (systolic or diastolic) is outside the rated range specified in part SPECIFICATIONS. In this case, you should consult a physician or check if your operation violated the instructions

The technical alarm condition (outside the rated range) is preset in the factory and cannot be adjusted or inactivated. This alarm condition is assigned as low priority according to IEC 60601-1-8. The technical alarm is non-latching and need no reset.


The signal displayed on LCD will disappear automatically after about 8 seconds.

# 6.13. Troubleshooting (1)

PROBLEM	POSSIBLE CAUSE	SOLUTION	
	The cuff position was not correct or it was not properly tightened	Apply the cuff correctly and try again	
LCD Display shows abnormal result	Body posture was not correct during testing	Review the "BODY POSTURE DURING MEASUREMENT" sections of the instructions and re-test	
	Speaking, arm or body movement, angry, excited or nervous during testing	Re-test when calm and without speaking or moving during the test	
	Irregular heartbeat (arrhythmia)	It is inappropriate for people with serious arrhythmia to use this Electronic Sphygmomanometer	

# POSSIBLE CAUSE | SOLUTION

LCD shows low battery symbol 🗓	Low Battery	Change the batteries

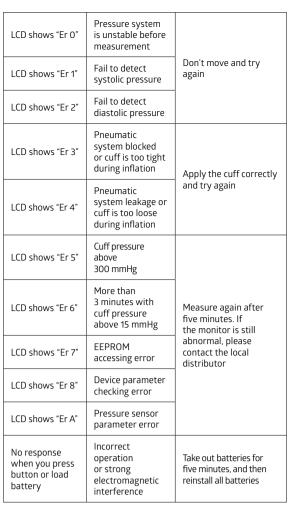

## 7. MAINTENANCE

- 2. Avoid high temperature and solarization
- Do not immerse the monitor in water as this will result in damage to the monitor
- 3. If this monitor is stored near freezing, allow it to acclimate to room temperature before use.
- disconnect the cuff from the monitor. 5. It is recommended the performance should be checked every
- squeezed well after moistened with water or diluted detergent.
- disinfected 2 times every week if needed (For example, in hospital or in clinic). Wipe the inner side (the side contacts skin) of the cuff by a soft cloth squeezed after moistened with a 3% solution of hydrogen
- . No component can be maintained by user in the monitor.
- cuff are resistant to disinfection with a 3% solution of hydrogen

## 8. SPECIFICATIONS

- 1. Product name: Wrist Blood Pressure Monitor,
- model: MED-57 2. Classification: Internally powered, Type BF applied part, IP22,
- No AP or APG, Continuous operation 3. Machine size: Approx. 73 mm × 62 mm × 28,5 mm (27/8" × 21/2" × 11/8")
- 6. Measuring method: Oscillometric method, automatic inflation
- Memory volume: 30 times with time and date stamp
- cuff pressure: 0-300 mmHg systolic: 60-280 mmHg diastolic: 20-199 mmHg,
- pressure: ±3 mmHg, pulse rate: ±5%.
- 13. Environmental temperature for storage and transport: -20°C~50°C (-4°F~122°F). 14. Environmental humidity for storage and transport: ≤85% RH.
- 16. Battery life: Approx 120 times. 17. Blood pressure monitor set:
- box 1 piece, a storage bag – 1 piece.

## 9. APPLIED STANDARDS

The digital automatic blood pressure monitor corresponds to the IEC 60601-1:2005/EN 60601-1:2006/AC:2010 (Medical electrical

IEC60601-1-2:2007/EN 60601-1-2:2007 /AC:2010 (Medical electrical equipment – Part 1-2: General requirements for basic safety and essential performance – Collateral standard: Electromagnetic compatibility - Requirements and tests),

EN 1060-1: 1995 + A1: 2002 + A2: 2009 (Non-invasive sphygmomanometers - Part 1: General requirements), EN 1060-3: 1997 + A1: 2005 + A2: 2009 (Non-invasive

- 1.  $\triangle$  Do not drop this monitor or subject it to strong impact.
- 4. △ Do not attempt to disassemble this monitor and do not
- 2 years or after it has been dropped. Please contact the service 6. Clean the monitor with a dry, soft cloth or a soft cloth
- 7 Keen the cuff clean. It is recommended the cuff should be
- peroxide, then dry the cuff by airing.
- 9. The external surfaces of the blood pressure monitors and the

- 4. Wrist cuff circumference: 13,5 cm 21,5 cm 5. Weight: not more than 69,3 g  $\pm$  10% (exclude batteries)
- and measurement
- 8. Power source: batteries: 2 ×1.5V === SIZE AAA 9. Measurement range:
- pulse rate: 40-200 beats/minute. 10. Accuracy:
- 11. Environmental temperature for operation: 10°C~40°C (50°F~104°F). 12. Environmental humidity for operation: ≤85% RH.
- 15. Environmental pressure: 80kPa-105kPa.
- blood pressure monitor 1 piece, wrist cuff – 1 piece. bladder – 1 piece, AAA batteries – 2 pieces, the instruction manual - 1 piece,
- **NOTE:** These specifications are subject to change without notice

equipment – Part 1: General requirements for basic safety and essential performance).

IEC 80601-2-30 : 2009+Cor.2010 (Medical electrical equipment -Part 2-30: Particular requirements for the basic safety and essential performance of automated non-invasive sphygmomanometers),

sphygmomanometers - Part 3: Supplementary requirements for electro-mechanical blood pressure measuring systems).

TYPE BF APPLIED PARTS (The cuff is type BF applied part)



10. SYMBOL INFORMATION



CE 0044 Certification OPERATING CONDITION



HOUSING INGRESS PROTECTION RATE: IP22 IP 22 (Protected from the penetration of solid bodies with dimension greater than 12 5 mm. Protected from the penetration of vertically falling water drops)

Warranty period is 3 years from the date of purchase for monitor and 1 year for cuff. This warranty doesn't cover any damages caused by improper using, and also battery, and packaging. When a manufacturing defect is revealed during the warranty period a faulty unit would be repaired or, if repairing is impossible, replaced with

### 12. ELECTROMAGNETIC COMPATIBILITY INFORMATION

The manufacturer may change units partially or completely if

Manufacturing date is in a serial number: WWYYXXXXX.

Electromagnetic

Immunity test levels

Professional healthcare facility

# Table 1 - Emission

necessary, without prior notice.

- Hellomenon	compliance	environment
RF emissions	CISPR 11	Home healthcare
KI elliissiolis	Group 1, Class B	environment
Harmonic distortion	IEC 61000-3-2	Home healthcare
	Class A	environment
Voltage fluctuations	IEC 61000-3-3	Home healthcare
and flicker	Compliance	environment
Table 2 – Enclosure Port		
		Immunity test levels

Phenomenon	Basic EMC standard	Immunity test levels Home Healthcare Environment
Electrostatic Discharge	IEC 61000-4-2	±8 kV contact ±2 kV, ±4 kV, ±8 kV, ±15 kV air
Radiated RF EM field	IEC 61000-4-3	10 V/m 80 MHz – 2.7 GHz 80% AM at 1k Hz
Proximity fields from RF wireless communications equipment	IEC 61000-4-3	Refer to table 3
Rated power frequency magnetic	IEC 61000-4-8	30 A/m

# Table 3 – Proximity fields from RF wireless communications

Band (MHz)

(MHz)		environment
385	380-390	Pulse modulation 18 Hz, 27 V/m
450	430-470	FM, ±5 kHz deviation, 1 kHz sine, 28 V/m
710		
745	704-787	Pulse modulation 217 Hz, 9 V/m
780		
810		
870	800-960	Pulse modulation 18 Hz, 28 V/m
930		
1720		
1845	1700-1990	Pulse modulation 217 Hz, 28 V/m
1970		
2450	2400-2570	Pulse modulation 217 Hz, 28 V/m
5240		
5500	5100-5800	Pulse modulation 217 Hz, 28 V/m
5785		
	•	

Last revision: 2020-W35




### B.Well Swiss AG, Bahnhofstrasse 24, 9443 Widnau, Switzerland

www.bwell-swiss.ch

THE OPERATION GUIDE MUST BE READ (The sign background colour: blue.The sign graphical symbol: white)

ENVIRONMENT PROTECTION -Waste electrical products should not be disposed of with household waste. Please recycle where facilities exist. Check with your local Authority or retailer for recycling



WARNING

REF SERIAL NUMBER SN



## 11. WARRANTY INFORMATION

## For all ME EQUIPMENT and ME SYSTEMS

equipment

Test

frequency